

Biotinylated Human CD200 R1/CRTR2 Protein

Cat. No. CD2-HM4R1B

Description

Source	Recombinant Biotinylated Human CD200 R1/CRTR2 Protein is expressed from HEK293 with His tag and Avi tag at the C-Terminus. It contains Ala27-Leu266.
Accession	AAQ19772
Molecular Weight	The protein has a predicted MW of 29.7 kDa. Due to glycosylation, the protein migrates to 52-70 kDa based on Bis-Tris PAGE result.
Endotoxin	Less than 1EU per µg by the LAL method.
Purity	> 95% as determined by Bis-Tris PAGE > 95% as determined by HPLC

Formulation and Storage


Formulation	Lyophilized from 0.22µm filtered solution in PBS (pH 7.4). Normally 8% trehalose is added as protectant before lyophilization.
Reconstitution	Centrifuge the tube before opening. Reconstituting to a concentration more than 100 µg/ml is recommended. Dissolve the lyophilized protein in distilled water.
Storage	-20 to -80°C for 12 months as supplied from date of receipt. -80°C for 3 months after reconstitution. Recommend to aliquot the protein into smaller quantities for optimal storage. Please minimize freeze-thaw cycles.

Background

CD200Fc, a chimeric molecule including the extracellular domain of CD200 and a murine IgG2a Fc region, regulates immune responses following engagement of a cell surface receptor, CD200R, expressed on cells of the myeloid and T cell lineage. A recent report focused attention on a family of CD200Rs, but concluded that only one member used CD200 as its ligand.


Assay Data

Bis-Tris PAGE

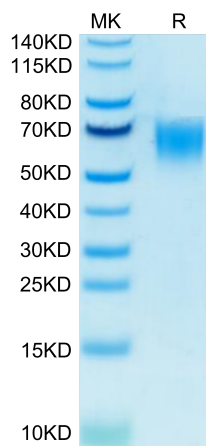

Biotinylated Human CD200 R1 on Bis-Tris PAGE under reduced condition. The purity is greater than 95%.

SEC-HPLC

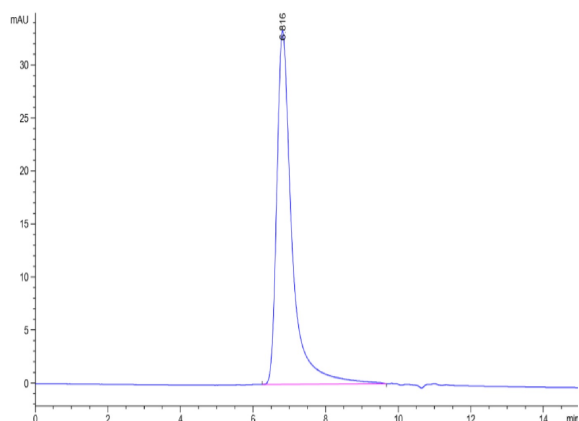


The purity of Biotinylated Human CD200 R1 is greater than 95% as determined by SEC-HPLC.

Assay Data

ELISA Data

Biotinylated Human CD200 R1, His Tag ELISA

0.1µg Biotinylated Human CD200 R1, His Tag Per Well

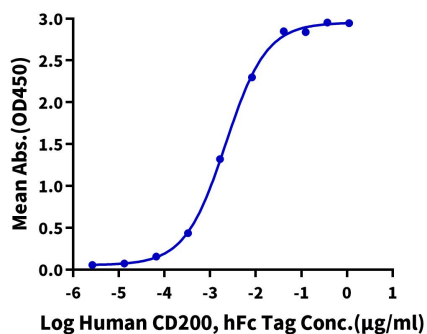

Immobilized Biotinylated Human CD200 R1, His Tag at 1µg/ml (100µl/well) on the streptavidin precoated plate (5µg/ml). Dose response curve for Human CD200, hFc Tag with the EC50 of 2.2ng/ml determined by ELISA (QC Test).